intensa™
by graham-field

560 SERIES EXAMINATION TABLE INSTALLATION AND OPERATION MANUAL

SAVE THIS MANUAL FOR FUTURE USE.

IN_560-INS-LAB-RevA26

CONTENTS

INTRODUCTION 3
INTENDED USE 3
CONTRAINDICATIONS 3
1 SAFETY PRECAUTIONS 4
SIGNIFICANCE OF SAFETY STATEMENTS 4
WARNINGS 4
ELECTROMAGNETIC COMPATIBILITY (EMC) INFORMATION 5
2 FEATURES 6
EXAM TABLE COMPONENT IDENTIFICATION 6
3 UNPACKING 7
UNPACKING THE EXAM TABLE 7
INSPECTION 7
4 INSTALLATION 8
INSTALLATION ELECTRICAL REQUIREMENTS 8
ELECTROMAGNETIC INTERFERENCE 8
LEVELING THE EXAM TABLE 9
ADDITIONAL ADJUSTMENTS / RELEVELING 9
5 OPERATION 10
OPERATION SAFETY 10
WEIGHT CAPACITY AND DUTY CYCLE 10
PERSONNEL CLEARANCE SAFETY 10
EQUIPMENT CLEARANCE SAFETY 10
560 EXAM TABLE HIGH-LOW OPERATION 11
USING THE HAND PENDANT 11
USING THE (OPTIONAL) FOOT CONTROL 11
EXAM TABLE HEIGHT RANGE 12
EXAM TABLE BACK ANGLE RANGE 12
PHYSICIAN'S ASSIST STORAGE CABINET 13
PATIENT LEGREST AND PROCEDURE TRAY 14
PATIENT ASSIST ARM 14
STIRRUP OPERATION 15
PELVIC TILT OPERATION 15
6 TROUBLESHOOTING 16
7 ROUTINE MAINTENANCE / CARE 17
MAINTENANCE 17
CLEANING 18
STORAGE 18
DISPOSAL 19
8 CERTIFICATION 19
9 SPECIFICATIONS 19
10 LIMITED WARRANTY 20
11 KEY TO SYMBOLS 21
12 APPENDIX 22
13 INDEX 27

INTRODUCTION

Congratulations on your purchase of the Intensa 560 Series Examination Table. The following pages will provide you with important safety and operating instructions on the installation and operation of the Examination Table, as well as maintenance and warranty information. Read this manual carefully before operating your Examination Table and refer to it as often as needed. Consult your authorized distributor and/or healthcare professional with any questions or concerns regarding safe and effective techniques for operating your Examination Table.

This guide covers the use of the Intensa 560 Series Examination Table. Keep in mind that the basic safety procedures included in this manual are to be used as a guide only. You may find it necessary to develop your own unique methods for safely utilizing the Examination Table. Again, consult your healthcare professionals for their recommendations and never hesitate to ask for their assistance.

Upon receipt of the Examination Table, inspect it closely to ensure that nothing is damaged, there are no loose or broken parts, that all Examination Table parts are in the proper place, etc. Immediately replace any worn or broken components. Your Examination Table should receive maintenance on a regular schedule and should be inspected frequently for proper operation. Contact Intensa Tech Support at 1.336.884.4096 with any maintenance concerns.

Info: *Before attempting to install the Examination Table, refer to the section titled "INSTALLATION" contained elsewhere in this manual. Contact Intensa Tech Support at 1.336.884.4096 or your Intensa authorized distributor if additional assistance is needed.*

Intended Use

The Intensa 560 Series Examination Table is intended to support patients during medical examinations. During these exams, medical professionals use adjusting mechanisms to manipulate and position the table to provide patient support and closer examination of a portion of or the entire patient.

This product has an expected service life of five (5) years.

To ensure the basic safety of the patient, the table is designed, tested, and evaluated to AAMI ES60601-1 wherein the essential performance in any single fault or combined fault condition is no unwanted movement of the table when in use.

Contraindications

⚠ **WARNING: This equipment is not suitable for use in the presence of highly flammable anesthetics or mixtures thereof and may result in serious injury or death.**

⚠ **WARNING: This equipment is not suitable for use in the presence of a highly oxygenated atmosphere and may result in serious injury or death.**

⚠ **WARNING: When a cauterization or high frequency surgical device is being used, the patient must be insulated from the metal table using a non-conductive material. Failure to do so could result in electrical shocks or burns to the patient.**

1 LIST OF WARNINGS AND CAUTIONS

⚠ **WARNING: Important! Read and understand these instructions before assembling or using the Intensa 560 Series Examination Table. If you do not understand any part of these warnings, cautions or instructions, contact a healthcare professional for direction in the use of this product. If the Intensa 560 Series Examination Table is not properly assembled, personal injury and damage to the 560 could result.**

Always consult your healthcare professional to determine safe methods most suitable for your individual abilities. Protect yourself, your attendant and Examination Table by having it serviced regularly. If you experience any malfunction, contact Intensa Tech Support at 1.336.884.4096 or your Intensa authorized distributor immediately, as a hazardous condition could result, causing personal injury or damage to your Examination Table.

Periodic inspection, adjustment and replacement of worn parts are necessary to provide years of excellent service. Refer to *CARE AND MAINTENANCE* section of this manual. Maintenance MUST be performed by qualified personnel ONLY.

SAVE THESE INSTRUCTIONS.

SIGNIFICANCE OF SAFETY STATEMENTS

Note the following special statements, used throughout this manual, and their significance:

⚠ **DANGER: Indicates a potential hazard situation or unsafe practice that, if not avoided, will result in death or serious personal injury.**

⚠ **WARNING: Indicates a potential hazard situation or unsafe practice that, if not avoided, could result in death or serious personal injury.**

⚠ **CAUTION: Indicates a potential hazard situation or unsafe practice that, if not avoided, could result in minor or moderate personal injury.**

▲ **NOTICE: Indicates a potential hazard situation or unsafe practice that, if not avoided, could result in product or property damage.**

Info: *Provides application recommendations or other useful information to ensure that you get the most from your product.*

WARNINGS — CAUTIONS AND PROPER OPERATION

⚠ **WARNING: If components are damaged or missing, contact your Intensa authorized distributor immediately. DO NOT use substitute parts. Use only Intensa replacement parts. The use of non-Intensa replacement parts could cause personal injury, property damage, and void the warranty.**

⚠ **WARNING: Unauthorized modification of your Examination Table could cause personal injury, property damage, and void the warranty.**

⚠ **WARNING: The Intensa 560 Series Examination Table maximum weight capacity is 600 lb (272 kg), EVENLY DISTRIBUTED. DO NOT exceed the maximum weight capacity.**

⚠ **WARNING: GF Health Products, Inc. ("GF") assumes no responsibility for any damage or injury caused by improper assembly or use of this product.**

⚠ **WARNING: Check all parts for shipping damage BEFORE using. In case of damage, DO NOT USE the equipment. Contact the carrier or your Intensa authorized distributor for further instructions.**

⚠ **WARNING: Unauthorized modification of the Examination Table or the use of non-Intensa replacement parts may change the structure of the table and could create a hazardous condition, which may result in serious injury and void the warranty.**

⚠ **WARNING: Ensure hand and foot controls remain clear when not in use to avoid unintended operation of the table.**

⚠ **WARNING: When the back of examination table is lowered, ensure hands or other objects are clear from the downward motion area.**

⚠ **WARNING: DO NOT allow the patient to operate the controls as they may not understand the operating control or have awareness of equipment or personnel clearances around the table, which can result in personal injury.**

⚠ **WARNING: If a malfunction occurs, immediately**

1. **Remove hand from hand control or remove foot from foot control,**
2. **Unplug the exam table power cord, and**
3. **Assist patient in getting off the table.**

⚠ **WARNING: Patient entry and egress should always be from the end of the seat when the table is at the lowest height to reduce chance of patient fall.**

⚠ **WARNING: GF Health Products, Inc. specifically disclaims responsibility for any bodily injury or property damage which may occur during any use which does not comply with federal, state or local laws or ordinances.**

ELECTROMAGNETIC COMPATIBILITY (EMC) INFORMATION

⚠ **WARNING: Medical Electrical Equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in this manual.**

⚠ **WARNING: Electronic equipment may be influenced by Radio Frequency (RFI). Caution should be exercised with regard to the use of portable communications in the area around such equipment. Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the Intensa equipment including specified Intensa equipment cables. Degradation of the performance of the Intensa equipment could result.**

⚠ **WARNING: If RFI causes erratic behavior, unplug the electric Intensa equipment immediately. Leave unplugged while transmission is in progress.**

⚠ **WARNING: The use of accessories, transducers, and cables other than those specified by the manufacturer may result in increased emissions or decreased immunity of the Intensa equipment. GF cables and accessories include motor cables, mains cable, pendant cables, and back up battery and cable.**

⚠ **WARNING: This equipment should not be used adjacent to or stacked with other equipment. If adjacent or stacked use with other equipment is necessary, this Intensa equipment and the other equipment should be observed to verify that they are operating normally.**

⚠ **WARNING: The EMISSIONS characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is usually required) this equipment might not offer adequate protection to radio frequency communication services. The user might need to take mitigation measures, such as relocating or reorienting the equipment.**

2 FEATURES

EXAM TABLE COMPONENT IDENTIFICATION

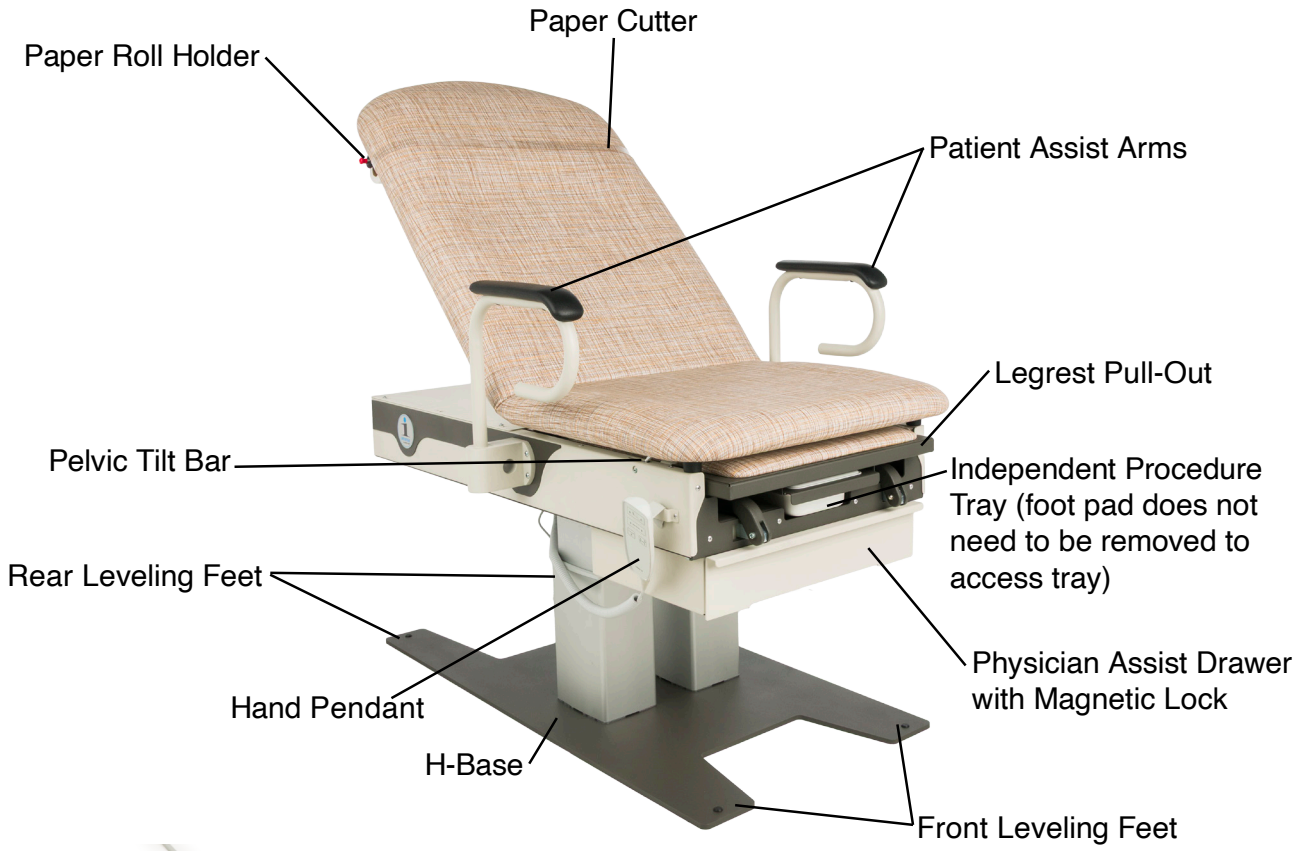

Optional Foot Control

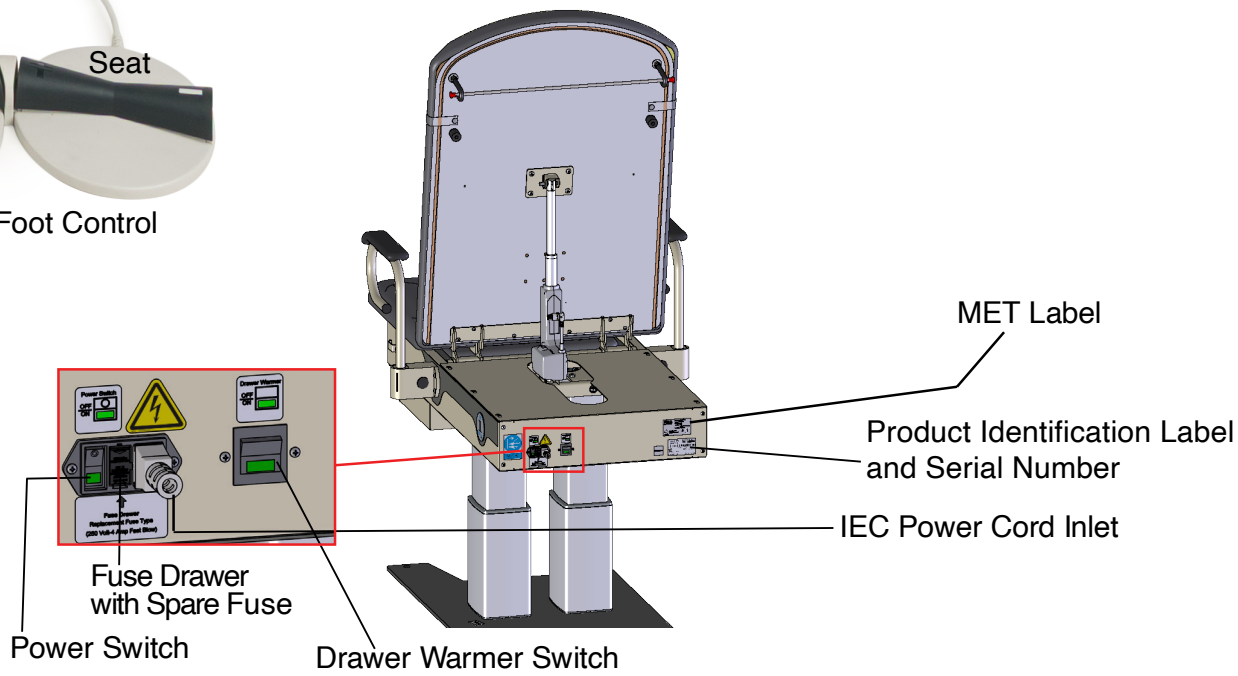

3 UNPACKING

UNPACKING THE EXAM TABLE

⚠ **WARNING: Because of weight, we recommend placing the exam table on a hand truck for transport to its installation location.**

▲ **NOTICE: DO NOT use a knife or other sharp object to open packaging — damage could occur to the exam table upholstery or surface.**

1. Check for any obvious damage to the carton or its contents. If damage is evident, notify the carrier or your Intensa authorized distributor.
2. Carefully remove external strapping and boxing.
3. Carefully remove blocking from shipping pallet that secures exam table to pallet.

▲ **NOTICE: DO NOT remove internal transport strapping from exam table until table is placed in final location; strapping will have labels denoting which straps should not be removed.**

⚠ **WARNING: DO NOT Use Stirrups, Legrest Pull-Out, or Upholstery to lift, move or slide the table. Personal injury and damage to exam table could occur.**

4. Once exam table is located in final position, remove internal transport strapping.

⚠ **WARNING: This exam table, as shipped, could weigh up to 315 lb (142.8 kg)— use sufficient personnel to lift and remove the exam table from the shipping pallet for placement into final location. DO NOT attempt to remove the exam table from the shipping pallet or move it without assistance. Use proper lifting technique; neglect of these procedures could result in serious injury.**

⚠ **WARNING: See illustration for proper lifting area.**

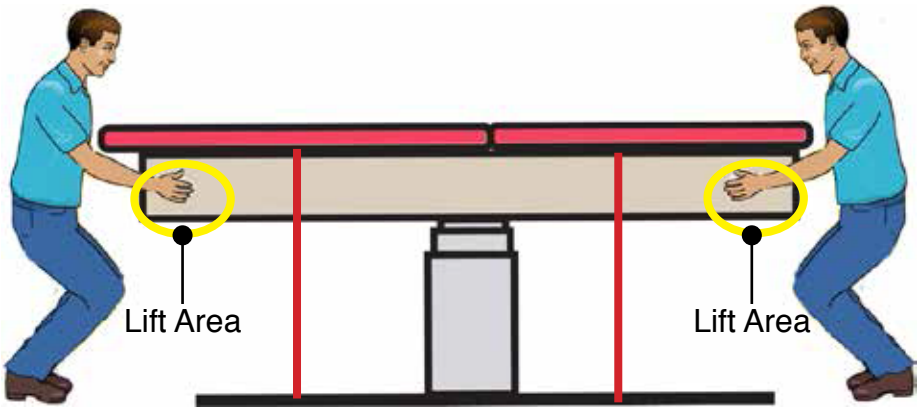

5. Carefully remove the exam table from the shipping pallet.

INSPECTION

1. Examine the Examination Table for nicks, dents, scratches or other damage. If damage is evident, notify the carrier or your Intensa authorized distributor.
2. Inspect all components.
3. If damage to any component is evident, notify the carrier or your Intensa authorized distributor.

4 INSTALLATION

⚠ **WARNING: DO NOT Use Stirrups, Legrest Pull-Out, or Upholstery to lift, move or slide the table. Personal injury and damage to exam table could occur. Lift only as described on previous page.**

INSTALLATION ELECTRICAL REQUIREMENTS

⚠ **WARNING: Use 115 VAC, 60 Hz. Failure to do so may result in electrical shock and may cause damage to the exam table.**

⚠ **WARNING: The power cord and table must be set up for easy access and use, with nothing obstructing the table from being unplugged.**

⚠ **WARNING: This table must only be connected to a mains supply with protective earth.**

⚠ **WARNING: When connecting equipment to a courtesy outlet, this creates a "Medical Electrical System" and which can result in a lowering of safety levels.**

⚠ **WARNING: No modifications, any changes to this equipment could result in serious injury or death.**

ELECTROMAGNETIC INTERFERENCE

This product is designed and built to minimize electromagnetic interference with other devices. If interference is noticed:

- Remove interfering device from the room.
- Plug exam table into an isolated circuit.

LEVELING THE EXAM TABLE

Tools required: *1/4" hex key, Flathead screwdriver*

fig. 5-1



Leveling Screw Caps

fig. 5-2



Leveling Screw Exposed

fig. 5-3

Leveling Screw Adjustment

1. Adjust all four leveling screws by using a 1/4" hex key to turn them clockwise (fig. 5-3). STOP when each screw touches the floor.
2. Insert the appropriate leveling screw caps (fig. 5-1) by aligning the cap with the hex in the leveling screw and applying light pressure until inserted.

   a. If minimal / no leveling was needed, use the shorter cap (fig. 5-1 left).

   b. If shorter cap doesn't reach the leveling screw, use the longer cap (fig. 5-1 right).

Note: *It's recommended to keep the unused caps in case additional adjustments are needed that impact the cap fit.*

For Additional Adjustments/Releveling After Moving Table

1. Locate leveling screw/caps on H-base leveling feet (4 total) (fig. 5-2).
2. Remove all four leveling screw caps by placing the screwdriver in the slot on the cap and gently lifting the cap. Leveling screws will now be exposed (fig. 5-2).
3. Adjust all four leveling screws by using a 1/4" hex key to turn them clockwise. STOP when each screw touches the floor (fig. 5-3).
4. Replace the leveling screw caps by aligning the cap with the hex in the leveling screw and applying light pressure until inserted.

Note: *Additional adjustments may need to be swapped to the longer cap if not in use initially.*

5 OPERATION

OPERATION SAFETY

Exam Table Weight Capacity and Duty Cycle

⚠ **WARNING: The Intensa 560 Series Examination Table maximum weight capacity is 600 lb (272 kg), EVENLY DISTRIBUTED. DO NOT exceed the maximum weight capacity.**

⚠ **WARNING: The Intensa 560 Series Examination Table Duty Cycle is 10%, or two minutes of use followed by eighteen minutes of nonuse.**

Personnel Clearance Safety

⚠ **WARNING: BEFORE each use of exam table, ensure personnel are clear of table. If personnel are not clear before any exam table functions are set in motion, personal injury could result.**

⚠ **WARNING: At lowest height, the top of the exam table is approximately 18 in. above the floor, and the bottom of the Physician's Assist Storage Cabinet is only 5.5 in. above the floor. Feet and legs must be clear from this area before lowering exam table.**

⚠ **WARNING: When the back of examination table is lowered, ensure hands or other objects are clear from the downward motion area.**

Equipment Clearance Safety

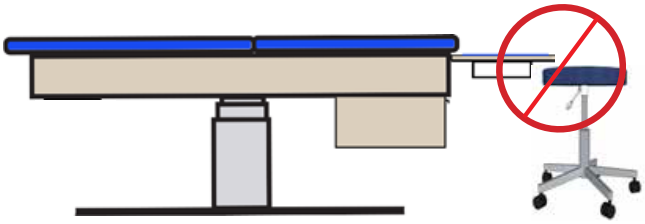

Ensure All Equipment is Clear of Table

⚠ **WARNING: Before each use of exam table, ensure all equipment is clear of table. If equipment is not clear before any exam table functions are set in motion, as shown above, personal injury and damage to equipment could result.**

⚠ **WARNING: If a malfunction occurs, immediately**

1. **Remove hand from hand control or remove foot from foot control,**
2. **Unplug the exam table power cord, and**
3. **Assist patient in getting off the table.**

⚠ **WARNING: Neglect to adhere to these instructions could result in patient injury or damage to the equipment.**

560 EXAM TABLE HIGH-LOW OPERATION

The exam table will stop once it reaches maximum or minimum height, whether operated with Hand Pendant Switch or Foot Control Switch.

Exam Table Height and Back Controls Using Hand Pendant

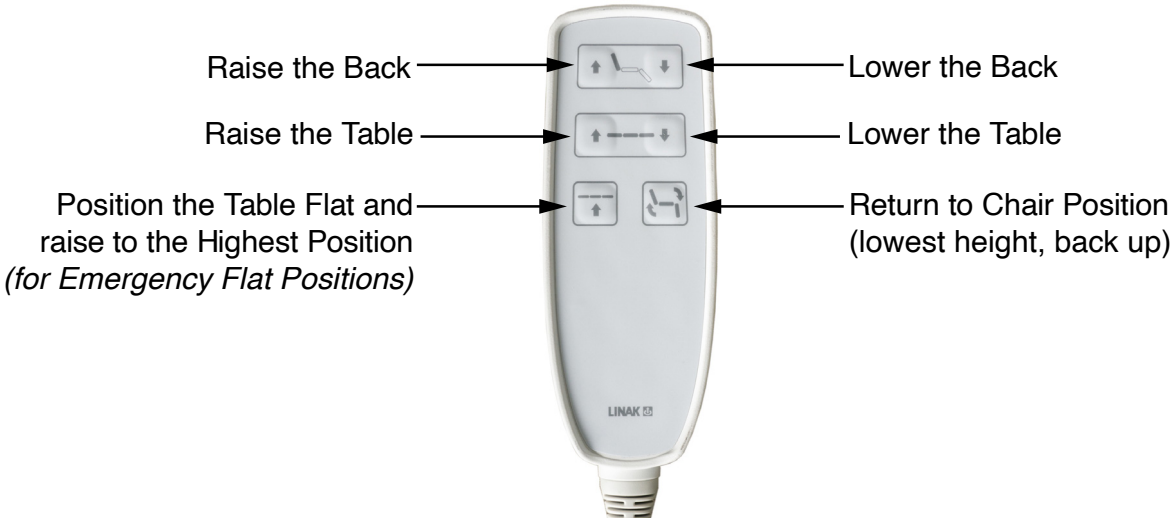

Hand Pendant Functions

Exam Table Height and Back Controls Using (Optional) Foot Control

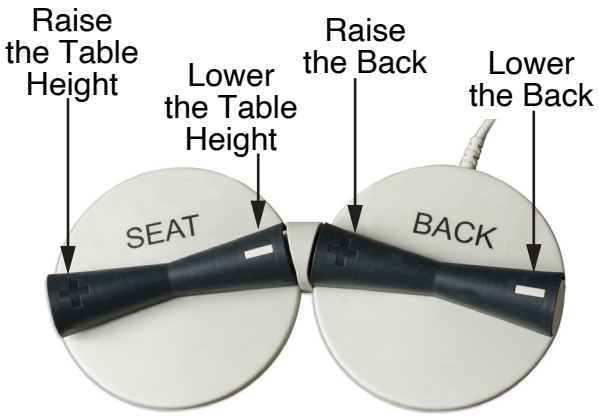

Foot Control Functions

Info: *The Foot Control will Not Control "Table Flat" or "Chair Position" Functions.*

⚠ **WARNING: Ensure hand and foot controls remain clear when not in use to avoid unintended operation of the table.**

⚠ **WARNING: DO NOT allow the patient to operate the controls as they may not understand the operating control or have awareness of equipment or personnel clearances around the table, which can result in personal injury.**

EXAM TABLE HEIGHT RANGE

⚠ **WARNING: Patient entry and egress should always be from the end of the seat when the table is at the lowest height to reduce chance of patient fall.**

This exam table is designed with a limit switch. Once the table reaches its maximum height or minimum height, vertical movements of the table will stop.

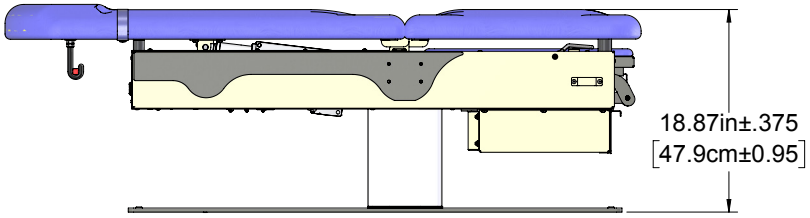

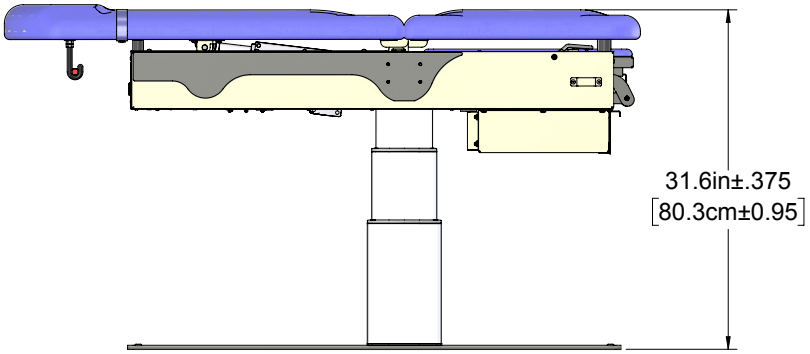

EXAM TABLE BACK ANGLE RANGE

This exam table is powered with manual control inputs used through pendant. Once the back reaches its maximum angle or a horizontal position, the back will stop moving.

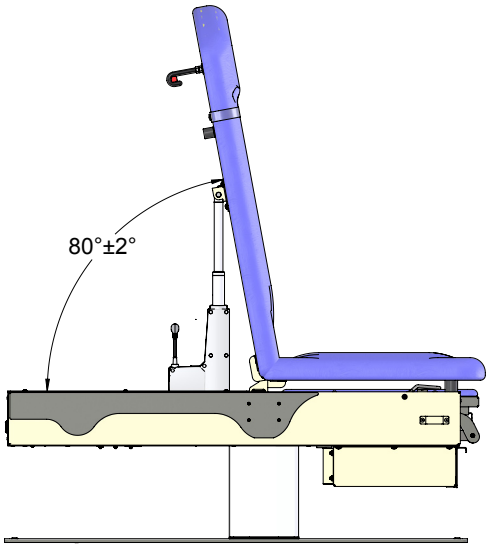

The exam table features a back angle of ~80˚ to help accommodate bariatric occupants comfortably, as shown above.

PHYSICIAN'S ASSIST STORAGE CABINET

▲ **NOTICE: The cabinet front can be used as a shelf. The maximum weight that can be supported is 10 lb (4.5 kg). The drawer front should not be lower than horizontal position; if drawer front is lower than horizontal position, DO NOT use drawer front as a shelf.**

The Physician's Assist Storage Cabinet has the following features:

- Dimensions, W x D x H: 20 in. x 12 in. x 4 in. (50.8 cm x 30.5 cm x 10.16 cm)
- Opening, W x H: 18 in. x 3.7 in. (45.7 cm x 9.4 cm)
- Usable Shelf Space, W x D: 20 in. x 12 in. (50.8 cm x 30.5 cm)
- Magnetic Lock with 12 in. (30.5 cm) continuous hinge for extra shelf support
- With optional Drawer Warmer W x D: 20 in x 11 in (50.8 cm x 27.9 cm)

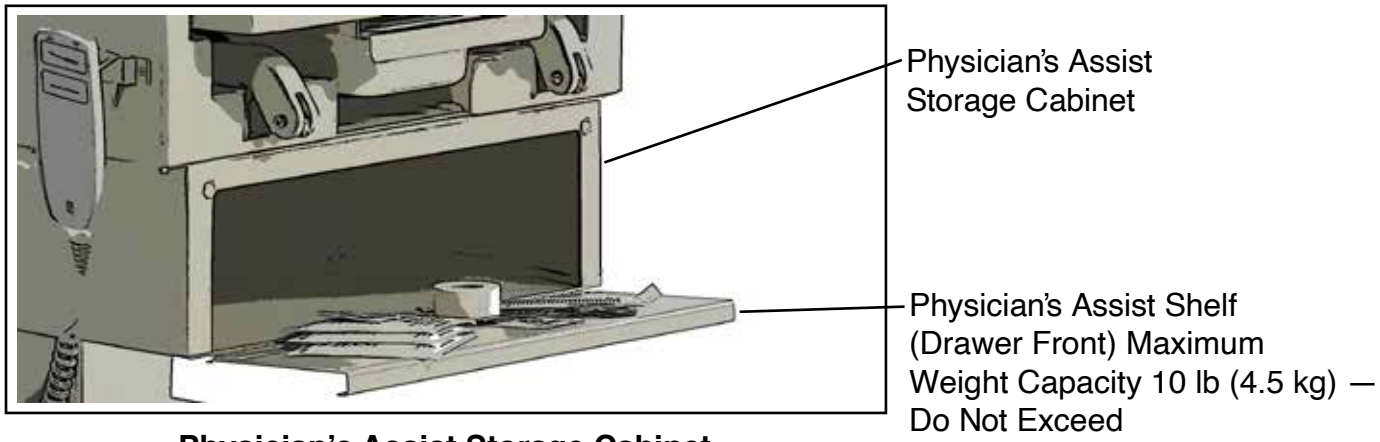

Physician's Assist Storage Cabinet

PATIENT LEGREST AND PROCEDURE TRAY

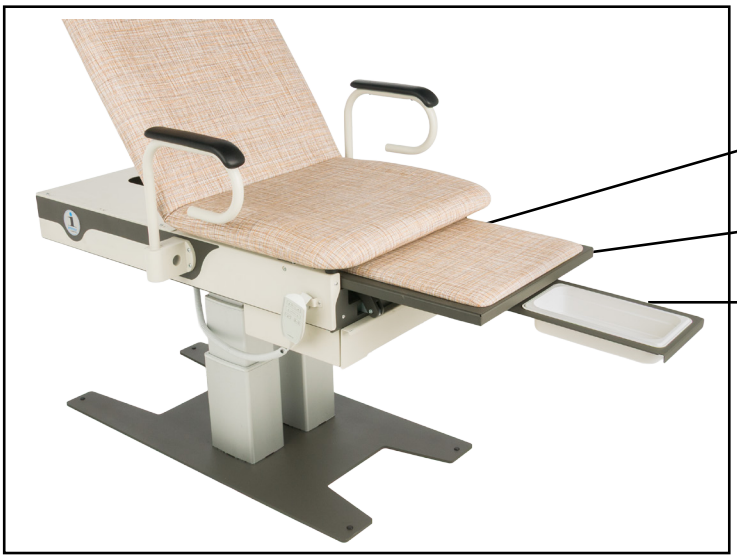

Patient Legrest and Procedure Tray

The Legrest Pull-Out, shown above, is located under the seat portion of the table cushion and can be extended approximately 13 in. (33 cm). The Procedure Tray or Treatment Pan can be extended up to 13.6 in. (33 cm) and can be used independently of the Legrest Pull-Out — the Legrest Pull-Out cushion need not be removed to access the Procedure Tray.

PATIENT ASSIST ARM

Forward Assist Arm Position

Outward Assist Arm Position

Rear Assist Arm Position

Refer to pictures above.

- Forward position is the normal Patient Assist Arm use position.
- Outward Position: Rotate Assist Arms 90 degrees outward by raising arms and turning them to outward position. To return to forward position, raise and rotate arms forward into brackets.
- Assist Arm Clearance: Rotate Assist Arms to rear position or totally remove for additional clearance.

STIRRUP OPERATION

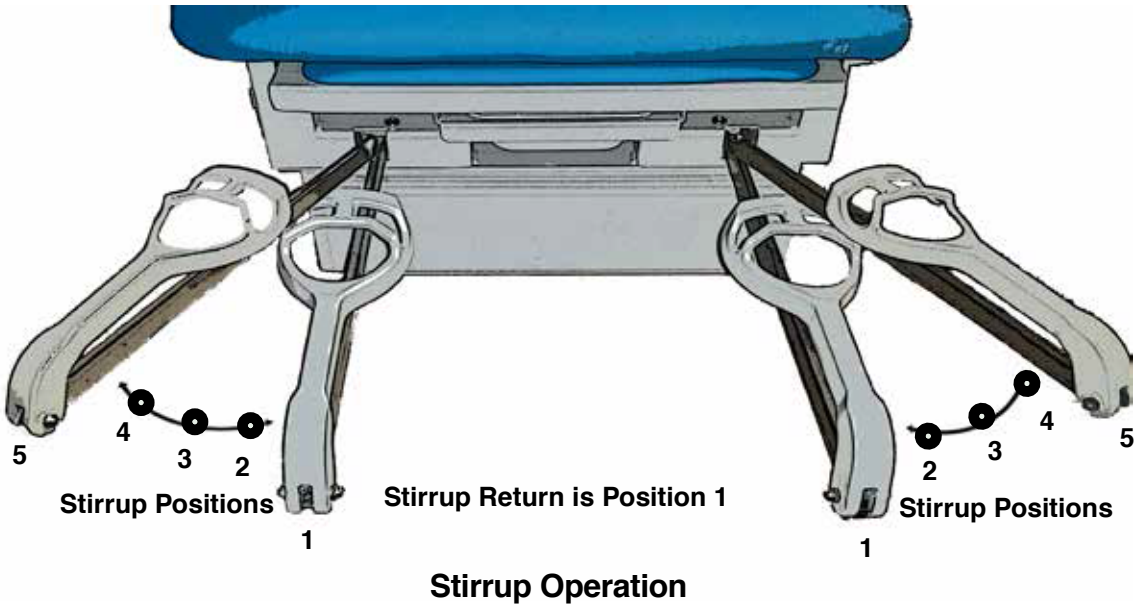

Stirrup Operation

⚠ **WARNING: Ensure stirrups are locked in place before use. Stirrups will not support entire patient weight (~100 lb weight limit).**

1. Pull Stirrup straight out and unfold heel portion.
2. To move stirrups left and right, lift slightly and move to desired location as shown above.
3. Press down to lock stirrup into one of the available five positions as shown above.

PELVIC TILT OPERATION

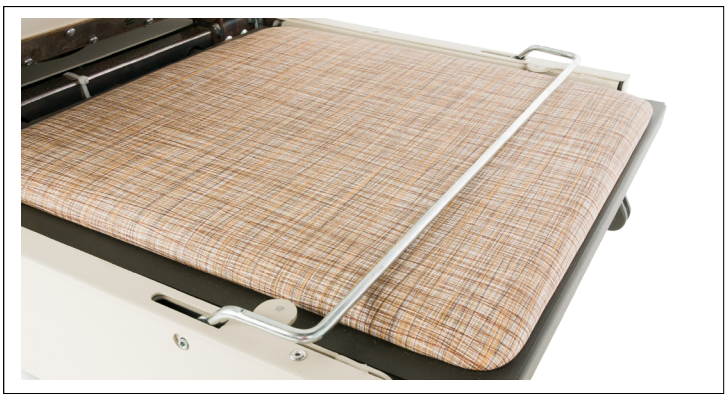

Pelvic Tilt Down Position

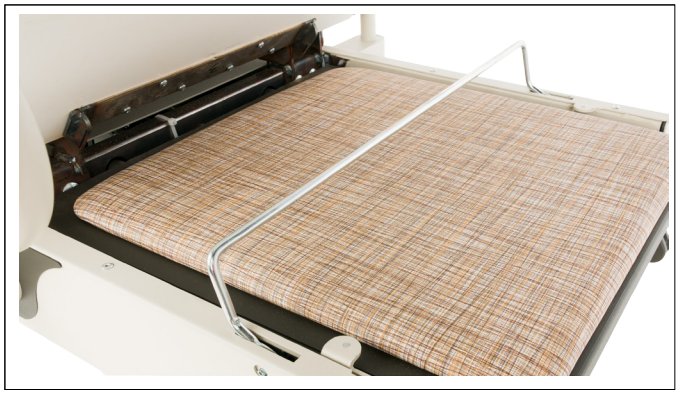

Pelvic Tilt Up Position

1. Lift seat portion of upholstery to raise and lower pelvic tilt.
2. Once pelvic tilt is in desired position, lower the seat.

6 TROUBLESHOOTING

⚠ **DANGER: SHOCK HAZARD — To reduce the risk of electric shock, unit is to be serviced by qualified service personnel ONLY.**

⚠ **DANGER: SHOCK HAZARD — ALWAYS disconnect the power source whenever troubleshooting or servicing any electric powered chair.**

⚠ **WARNING: DO NOT attempt to repair components or parts on your exam table, as this may invalidate your warranty or cause further problems that may result in patient injury. Stop using your exam table immediately if it is not functioning correctly.**

The following list of problems and their solutions will assist you in determining what may be causing your exam table not to function as designed.

If	Then
Nothing moves	**Step 1:** Ensure the exam table is connected to power and the green indicator light on the top of the power supply is on. **Step 2:** Plug unit into a mains supply wall receptacle and observe the control box LED: • If the control box LED is off, replace the control box. • If the control box LED illuminates, check the pendant cable connection at the control box. • Replace pendant if necessary.
Audible beeping error signal is heard, nothing moves	A function that is faulty or has lost motor position will cause the Control Box to beep intermittently when the faulty function's Hand Control Pendant button is depressed. All buttons depressed after the error function will also be non-functional and will cause a Control Box beep. If table requires more than 4 Amps to raise, movement will stop and the control box will begin beeping due to current overload. **Step 1:** Simultaneously press and hold the table up and down buttons (the Control Box should start beeping) for approximately five seconds until beeping stops. **Step 2:** Reinitialize the motors by: • Lowering the head deck with the head down button. • Lowering the table height with the table down button. **Note:** *If an audible error beep occurs again during reset lowering of a function or while checking functionality, the function that initiated the beep is faulty. Contact Intensa Tech Support if this occurs.* **Note:** *Lowering of the motors will reset the system and should resolve minor synchronization or position lost issues.* **Step 3:** Check the table functionality.
Unusual sounds or uneven movement during operation	Stop the actuator system immediately if anything unusual is observed. Check for any obstructions. If issue persists, call Intensa Tech Support at 1.336.884.4096.
Unusual noises or electrical smells	Switch off the mains voltage immediately and the external battery, if any. Call Intensa Tech Support at 1.336.884.4096.

⚠ **WARNING: If you experience a problem with your exam table and are unable to service it yourself, contact Intensa Tech Support at 1.336.884.4096.**

⚠ **WARNING: The exam table electronic system contains no serviceable parts. DO NOT open the motors, cables, or pendant hand control. ONLY an Intensa authorized distributor or factory-trained personnel may perform service or adjustments on these components.**

Contact Intensa Tech Support at 1.336.884.4096 for additional information required to service or repair the equipment.

7 ROUTINE MAINTENANCE / CARE

MAINTENANCE

⚠ **WARNING: Service and repair of the Intensa 560 Series Examination Table MUST be performed by qualified personnel ONLY.**

⚠ **WARNING: Unauthorized modification of the Examination Table or the use of non-Intensa replacement parts may change the structure of the table and could create a hazardous condition, which may result in serious injury and void the warranty.**

Info: *For more detailed information, please contact Intensa Tech Support at 1.336.884.4096.*

Note: *The manufacturer will provide the appropriate circuit diagrams, component parts lists, descriptions, and calibration instructions to assist qualified service personnel in parts repair.*

Have a qualified service technician perform the following maintenance as scheduled:

Maintenance Procedure	Materials / Action Required	Schedule
Inspect all mechanical functions for good operation.	If replacement is needed, contact Intensa Tech Support at 1.336.884.4096.	Every 3 months
Examine power cord for wear and function.	Examine for external wear, cuts, or wear. If replacement is needed, contact Intensa Tech Support at 1.336.884.4096.	
Inspect all fasteners to ensure proper fit, position and tightness (including nuts, bolts, etc.).	Proper size wrench and screwdriver	
Lubricate all moving and sliding parts and hinge points.	Lithium grease	
Inspect all surfaces and remove any sharp or burred areas; apply touch-up paint where required.	Metal file, proper color paint (specify color when ordering)	

⚠ **WARNING: After performing maintenance, if you believe a component or part is not functioning properly, immediately contact Intensa Tech Support at 1.336.884.4096, as a potentially hazardous condition could exist.**

CLEANING

▲ **NOTICE: DO NOT wash Examination Table under water pressure or steam clean.**

▲ **NOTICE: Cleaning solvents, dyes or sharp objects can damage upholstery. Promptly remove any excess fluids and rinse surface with clean water and wipe surface dry. For basic cleaning use mild soap and water, rinse thoroughly and wipe surface dry.**

Perform the following cleaning procedures as scheduled:

	Cleaning Procedure	Schedule	Cleaning Agent *	Special Notes
Pads	Wipe with damp cloth to remove any foreign material.	After each use	Routine hospital grade disinfectants, soap and water.	Use only medium strength cleaners Do not steam clean or pressure wash.
Exam table	Wipe with damp cloth to remove any foreign material.	After each use	Routine hospital grade disinfectants, soap and water.	Lubricate pivot points after cleaning.
Electrical	Wipe external surfaces ONLY with damp cloth to remove any foreign material.	After each use	Routine hospital grade disinfectants, soap and water.	Use only medium strength cleaners.

* Disinfecting and Cleaning Upholstery - ALWAYS follow manufacturer's recommended dilution	
Disinfectants for vinyl products	Phenolic disinfectants are the best choice for vinyl.
	Properly diluted quaternaries are also acceptable for vinyl.
	Quaternary / Isopropyl disinfectants ARE NOT recommended for vinyl.
Disinfectants for urethane products	Quaternary disinfectants are recommended for urethane.
	Quaternary / Isopropyl disinfectants are recommended for urethane.
	Phenolics SHOULD BE AVOIDED on urethane.
Disinfectants for all products	All fabrics may be cleaned with a 1:10 dilution of household bleaches containing 5.25% sodium hypochlorite as recommended by the Centers for Disease Control in Atlanta, Georgia; there is no harmful effect on the fabric.
	Disinfectants applied at full concentration or in highly concentrated solutions will decrease the useful life of fabric.
	Iodophor-type disinfectants used on fabric may result in staining.
Soils or Stains	Use neutral soapsuds and lukewarm water; DO NOT use harsh cleansers, solvents or detergents.
Hard-To-Clean Spots	Use standard household / vinyl cleansers and a soft bristle brush on troublesome spots or stains; presoak heavy, dried-on soil.
Laundering	**Laundering Vinyl-laminated, Polyurethane-coated, or Rubber-coated fabric IS NOT recommended;** laundering may substantially decrease the useful life of the fabric.

STORAGE

Store the repackaged Examination Table in a dry area.

DISPOSAL

⚠ **WARNING: During normal use of this product, it could become contaminated and may present a biohazard to waste sites.**

This product may contain substances that could be harmful to the environment if disposed of in places (landfills) that are not appropriate according to local legislation.

At the end of this product's useful life, dispose of it in accordance with local requirements, or contact the manufacturer for advice. Recycle this product through your recycling facility or dispose of it in accordance with local regulations.

We recommend disassembling and dividing the equipment and components into different waste groups such as: metal, cable, electronic, recoverable resource and plastic for recycling or combustion. Most plastic components are provided with a plastic types code and fiber content to aid sorting of plastic parts.

8 CERTIFICATION

Certification	AAMI ES60601-1

9 SPECIFICATIONS

Exam Table Load Rating (Evenly Distributed)		600 lb (272 kg)
Legrest Support Maximum Weight Capacity		50 lb (23 kg)
Patient Assist Arm Maximum Weight Capacity		100 lb (46 kg)
Table Height Range		18.8" to 31.6" ± .375" (47.8 cm to 80.3 cm ± .95 cm)
Back Angle Range		0° to 80° ± 2°
Upholstered Top Size (W x L)		27"x 59" ± 1" (69 cm x 149 cm ± 2.54 cm)
Upholstered Leg Support Pad Size (W x L)		18" x 19.5" (46 cm x 49.5 cm)
COM (Customer's Own Material) Requirements		3 yd. (2.74 m)
Overall Exam Table Length		59" ± 1" (149 cm ± 2.54 cm)
Overall Exam Table Length with Leg Extension		71.6" ± 1"(181.8 cm ± 2.54 cm)
Storage Cabinet (W x L x D)		12" x 20" x 4" (30.4 cm x 50.8 cm x 10 cm)
Electrical Requirements	Models 560, 560-PS, 560-DW, 560-FL	115-120 VAC Drawer warmer 120 VAC
Power Cord	Length (from table)	144" (365.7 cm)
	Specifications	300V / 16AWG/ 3 Conductor / SJT Jacket with Hospital Grade Plug Detachable Power Cord
Foot Switch Ingress Against Liquid		IPX6
Drawer Warmer (optional) temperature		Will heat area approximately 90°
Paper Roll Sizes (W x Roll Diameter)		18 in. x 3 in. (46 cm x 8 cm)
		19 in. x 3 in. (48 cm x 8 cm)
		21 in. x 3 in. (53 cm x 8 cm)
Transport and Storage Conditions	Temperature Range	-14°F to 122°F (-10°C to 50°C)
	Relative Humidity	20% to 90% at 30°C non-condensing
Operating Conditions	Temperature Range	41°F to 104°F (5°C to 40°C)
	Relative Humidity	20% to 90% at 30°C non-condensing
Fuses		10 Amp / 250 VAC Fast Blow

10 LIMITED WARRANTY

SCOPE OF WARRANTY

Intensa, inc. ("Intensa") warrants to the original purchaser only that it will replace or repair components, at Intensa's sole discretion, that are defective in material or workmanship under normal use and service. All warranties are conditioned upon the proper use of the products strictly in accordance with good commercial practice and applicable Intensa instructions and manuals, including proper use and maintenance. To the extent that a third party warrants a component, Intensa conveys all of its rights under that warranty to the original purchaser, to the extent permitted.

This limited warranty shall only apply to defects that are reported in accordance with the provisions set forth in this warranty document, within the applicable warranty period and which, upon examination by Intensa or its authorized representative, prove to be a warranty item. (See Obtaining Warranty Service below) This limited warranty is not transferable.

Within the guidelines set forth in this document, the warranted components and time periods are set forth below:

EXAMINATION TABLE COMPONENTS *

Base:.....five (5) years
Mechanical Components:.....three (3) years
Electronic Components:.....two (2) years
Original and Replacement Upholstered Tops ǂ: .....one (1) year
Replacement Parts ǂ:.....ninety (90) days

* Labor is not included in the warranty.

ǂ Upholstery is only warranted on material supplied by Intensa .

ǂ The warranty period is as designated above. If a part is replaced under warranty, the original warranty period will not be affected. All other replacement parts will be subject to the warranty period specified.

The applicable warranty period shall commence from date of shipment to the original customer, unless there is an expiration date on the component in which case the warranty shall expire on the earlier of warranty period or the expiration date.

OBTAINING WARRANTY SERVICE

This limited warranty shall only apply to defects that are reported to the Distributor from whom the Customer purchased the product within the applicable warranty period. If there is not a Distributor, you must contact Intensa directly by calling 1.336.884.4096, or by e-mailing a request to Intensa @grahamfield.com. Specific directions will be provided by the Customer Service Representative. Failure to abide by the specific directions will result in denial of the warranty claim.

EXCLUSIONS

The warranty does not cover and Intensa shall not be liable for the following:

1) Defects, damage, or other conditions caused, in whole or in part, by misuse, abuse, negligence, alteration, accident, freight damage, tampering or failure to seek and obtain repair or replacement in a timely manner;
2) Products which are not installed, used, or properly cleaned and maintained as required in the official manual for the applicable product;
3) Products considered to be of a non-durable nature including, but not limited to: filters, fuses, gaskets, lubricants, and charts;
4) Accessories or parts not provided by Intensa ;
5) Matching of color, grain or texture except to commercially acceptable standards;
6) Changes in color caused by natural or artificial light:
7) Charges by anyone for adjustments, repairs, replacement parts, installation or other work performed upon or in connection with such products which are not expressly authorized in writing, in advance, by Intensa ;
8) Any labor or shipping charges incurred in the replacement part installation or repair;
9) Costs and expenses of regular maintenance and cleaning; and
10) Representations and warranties made by any person or entity other than Intensa .

ENTIRE WARRANTY, EXCLUSIVE REMEDY AND CONSEQUENTIAL DAMAGES DISCLAIMER

THIS WARRANTY IS INTENSA'S ONLY WARRANTY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED. INTENSA MAKES NO IMPLIED WARRANTIES OF ANY KIND INCLUDING ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. IF ANY MODEL OR SAMPLE WAS SHOWN TO THE CUSTOMER, SUCH MODEL OR SAMPLE WAS USED MERELY TO ILLUSTRATE THE GENERAL TYPE AND QUALITY OF THE PRODUCT AND NOT TO REPRESENT THAT THE PRODUCT WOULD NECESSARILY CONFORM TO THE MODEL OR SAMPLE IN ALL RESPECTS. THIS WARRANTY IS LIMITED TO THE REPAIR OR REPLACEMENT OF THE DEFECTIVE PARTS. INTENSA SHALL NOT BE LIABLE FOR AND HEREBY DISCLAIMS ANY DIRECT, SPECIAL, INDIRECT, INCIDENTAL, EXEMPLARY OR CONSEQUENTIAL DAMAGES, INCLUDING, BUT NOT LIMITED TO: DAMAGES FOR LOSS OF PROFITS OR INCOME, LOSS OF USE, DOWNTIME, COVER, OR EMPLOYEE OR INDEPENDENT CONTRACTOR WAGES, PAYMENTS AND BENEFITS. CERTAIN STATES MAY CONFER ADDITIONAL RIGHTS REGARDING WARRANTIES AND IN THOSE STATES INTENSA'S LIABILITY AND THE LIABILITY OF INTENSA'S SUPPLIERS, SHALL BE LIMITED TO THE FULLEST EXTENT PERMITTED BY LAW.

The warranties contained herein, together with Intensa's current Terms and Conditions, contain all the representations and warranties with respect to the subject matter of this document, and supersede all prior negotiations, agreements and understandings with respect thereto. The recipient of this document hereby acknowledges and represents that it has not relied on any representation, assertion, guarantee, warranty, collateral contract or other assurance, except those set out in this document.

For additional information on this product or this warranty, please contact an Intensa Customer Service Representative.

NOTES:

1) Additional terms and conditions may apply. See Intensa's General Terms and Conditions on its website and the specific warranties, which may accompany the specific product.
2) Freight claims must be notated on the appropriate shipping documents and must be made with immediacy. International, federal and state regulations govern specific requirements for freight claims. Failure to abide by those regulations may result in a denial of the freight claim. Intensa will assist you in filing the freight claim.
3) Claims for any short shipment must be made within three (3) days of the invoice date.

11 KEY TO SYMBOLS

The following symbols are used on Intensa product labels.

Symbol	Meaning
	Protective Earth
	General Warning Sign
	Shock Hazard
CLASSIFIED MET US	MET
	Disconnect before Service
MD	Medical Device
	Manufacturer

Symbol	Meaning
	Follow Instructions for Use
	Type B Applied Part
UDI	Unique Device Identifier
SN	Serial Number

12 APPENDIX

12.1 GUIDANCE AND MANUFACTURER'S DECLARATION — ELECTROMAGNETIC EMISSIONS

The Intensa 560 Series Examination Table is intended for use in the electromagnetic environment specified below. The customer or the user of the Intensa 560 Series Examination Table should assure that it is used in such an environment.		
Emissions Test	**Compliance**	**Electromagnetic Environment — Guidance**
RF emissions CISPR 11	Group 1	The Intensa 560 Series Examination Table uses RF energy only for its internal function. Therefore, its RF emission is very low and are not likely to cause any interference in nearby electronic equipment. The Intensa 560 Series Examination Table is suitable for use in all establishments other than domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
RF emissions CISPR 11	Class A	
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations / flicker emissions IEC 61000-3-3	Complies	

12.2 ENCLOSURE PORT[1]

Phenomenon	Basic EMC standard or test method	IMMUNITY TEST LEVELS
		Professional healthcare facility environment
ELECTROSTATIC DISCHARGE	IEC 61000-4-2	± 8 kV contact ± 2 kV, ± 4 kV, ± 8 kV, ± 15 kV air
Radiated RF EM fields [a)]	IEC 61000-4-3	3 V/m [f)] 80 MHz – 2,7 GHz [b)] 80 % AM at 1 kHz [c)]
Proximity fields from RF wireless communications equipment	IEC 61000-4-3	See Table 9.3.
RATED power frequency magnetic fields [d) e)]	IEC 61000-4-8	30 A/m [g)] 50 Hz or 60 Hz

a) The interface between the PATIENT physiological signal simulation, if used, and the ME EQUIPMENT or ME SYSTEM shall be located within 0,1 m of the vertical plane of the uniform field area in one orientation of the ME EQUIPMENT or ME SYSTEM.

b) ME EQUIPMENT and ME SYSTEMS that intentionally receive RF electromagnetic energy for the purpose of their operation shall be tested at the frequency of reception. Testing may be performed at other modulation frequencies identified by the RISK MANAGEMENT PROCESS. This test assesses the BASIC SAFETY and ESSENTIAL PERFORMANCE of an intentional receiver when an ambient signal is in the passband. It is understood that the receiver might not achieve normal reception during the test.

c) Testing may be performed at other modulation frequencies identified by the RISK MANAGEMENT PROCESS.

d) Applies only to ME EQUIPMENT and ME SYSTEMS with magnetically sensitive components or circuitry.

e) During the test, the ME EQUIPMENT or ME SYSTEM may be powered at any NOMINAL input voltage, but with the same frequency as the test signal (see Table 1).

f) Before modulation is applied.

g) This test level assumes a minimum distance between the ME EQUIPMENT or ME SYSTEM and sources of power frequency magnetic field of at least 15 cm. If the RISK ANALYSIS shows that the ME EQUIPMENT or ME SYSTEM will be used closer than 15 cm to sources of power frequency magnetic field, the IMMUNITY TEST LEVEL shall be adjusted as appropriate for the minimum expected distance.

12.3 ENCLOSURE PORT IMMUNITY TO RF WIRELESS COMMUNICATIONS EQUIPMENT [1]

Test frequency (MHz)	Band [a)] (MHz)	Service [a)]	Modulation [b)]	Maximum power (W)	Distance (m)	IMMUNITY TEST LEVEL (V/m)
385	380 –390	TETRA 400	Pulse modulation [b)] 18 Hz	1,8	0,3	27
450	430 – 470	GMRS 460, FRS 460	FM [c)] ± 5 kHz deviation 1 kHz sine	2	0,3	28
710	704 – 787	LTE Band 13, 17	Pulse modulation [b)] 217 Hz	0,2	0,3	9
745						
780						
810	800 – 960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation [b)] 18 Hz	2	0,3	28
870						
930						
1 720	1 700 – 1 990	GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3, 4, 25; UMTS	Pulse modulation [b)] 217 Hz	2	0,3	28
1 845						
1 970						
2 450	2 400 – 2 570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation [b)] 217 Hz	2	0,3	28
5 240	5 100 – 5 800	WLAN 802.11 a/n	Pulse modulation [b)] 217 Hz	0,2	0,3	9
5 500						
5 785						

12.4 INPUT AC POWER PORT [1]

Phenomenon	Basic EMC standard	IMMUNITY TEST LEVELS
		Professional healthcare facility environment
Electrical fast transients / bursts [a) l) o)]	IEC 61000-4-4	± 2 kV 100 kHz repetition frequency
Surges [a) b) j) o)] Line-to-line	IEC 61000-4-5	± 0,5 kV, ± 1 kV
Surges [a) b) j) k) o)] Line-to-ground	IEC 61000-4-5	± 0,5 kV, ± 1 kV, ± 2 kV
Conducted disturbances induced by RF fields [c) d) o)]	IEC 61000-4-6	3 V [m)] 0,15 MHz – 80 MHz 6 V [m)] in ISM bands between 0,15 MHz and 80 MHz [n)] 80 % AM at 1 kHz [e)]
Voltage dips [f) p) r)]	IEC 61000-4-11	0 % U_T; 0,5 cycle [g)] At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315° [q)]
		0 % U_T; 1 cycle and 70 % U_T; 25/30 cycles [h)] Single phase: at 0°
Voltage interruptions [f) i) o) r)]	IEC 61000-4-11	0 % U_T; 250/300 cycle [h)]

a) The test may be performed at any one power input voltage within the ME EQUIPMENT or ME SYSTEM RATED voltage range. If the ME EQUIPMENT or ME SYSTEM is tested at one power input voltage, it is not necessary to re-test at additional voltages.

b) All ME EQUIPMENT and ME SYSTEM cables are attached during the test.

c) Calibration for current injection clamps shall be performed in a 150 Ω system.

d) If the frequency stepping skips over an ISM or amateur band, as applicable, an additional test frequency shall be used in the ISM or amateur radio band. This applies to each ISM and amateur radio band within the specified frequency range.

e) Testing may be performed at other modulation frequencies identified by the RISK MANAGEMENT PROCESS.

f) ME EQUIPMENT and ME SYSTEMS with a d.c. power input intended for use with a.c.-to-d.c. converters shall be tested using a converter that meets the specifications of the MANUFACTURER of the ME EQUIPMENT or ME SYSTEM. The IMMUNITY TEST LEVELS are applied to the a.c. power input of the converter.

g) Applicable only to ME EQUIPMENT and ME SYSTEMS connected to single-phase a.c. mains.

h) E.g. 10/12 means 10 periods at 50 Hz or 12 periods at 60 Hz.

i) ME EQUIPMENT and ME SYSTEMS with RATED input current greater than 16 A / phase shall be interrupted once for 250/300 cycles at any angle and at all phases at the same time (if applicable). ME EQUIPMENT and ME SYSTEMS with battery backup shall resume line power operation after the test. For ME EQUIPMENT and ME SYSTEMS with RATED input current not exceeding 16 A, all phases shall be interrupted simultaneously.

12.4 CONTINUED

j) ME EQUIPMENT and ME SYSTEMS that do not have a surge protection device in the primary power circuit may be tested only at ± 2 kV line(s) to earth and ± 1 kV line(s) to line(s).

k) Not applicable to CLASS II ME EQUIPMENT and ME SYSTEMS.

l) Direct coupling shall be used.

m) r.m.s., before modulation is applied.

n) The ISM (industrial, scientific and medical) bands between 0,15 MHz and 80 MHz are 6,765 MHz to 6,795 MHz; 13,553 MHz to 13,567 MHz; 26,957 MHz to 27,283 MHz; and 40,66 MHz to 40,70 MHz. The amateur radio bands between 0,15 MHz and 80 MHz are 1,8 MHz to 2,0 MHz, 3,5 MHz to 4,0 MHz, 5,3 MHz to 5,4 MHz, 7 MHz to 7,3 MHz, 10,1 MHz to 10,15 MHz, 14 MHz to 14,2 MHz, 18,07 MHz to 18,17 MHz, 21,0 MHz to 21,4 MHz, 24,89 MHz to 24,99 MHz, 28,0 MHz to 29,7 MHz and 50,0 MHz to 54,0 MHz.

o) Applicable to ME EQUIPMENT and ME SYSTEMS with RATED input current less than or equal to 16 A / phase and ME EQUIPMENT and ME SYSTEMS with RATED input current greater than 16 A / phase.

p) Applicable to ME EQUIPMENT and ME SYSTEMS with RATED input current less than or equal to 16 A / phase.

q) At some phase angles, applying this test to ME EQUIPMENT with transformer mains power input might cause an overcurrent protection device to open. This can occur due to magnetic flux saturation of the transformer core after the voltage dip. If this occurs, the ME EQUIPMENT or ME SYSTEM shall provide BASIC SAFETY during and after the test.

r) For ME EQUIPMENT and ME SYSTEMS that have multiple voltage settings or auto ranging voltage capability, the test shall be performed at the minimum and maximum RATED input voltage. ME EQUIPMENT and ME SYSTEMS with a RATED input voltage range of less than 25 % of the highest RATED input voltage shall be tested at one RATED input voltage within the range. See Table 1 Note c) for examples calculations.

12.5 PATIENT COUPLING PORT [1]

Phenomenon	Basic EMC standard	IMMUNITY TEST LEVELS
		Professional healthcare facility environment
ELECTROSTATIC DISCHARGE [c)]	IEC 61000-4-2	± 8 kV contact ± 2 kV, ± 4 kV, ± 8 kV, ± 15 kV air
Conducted disturbances induced by RF fields [a)]	IEC 61000-4-6	3 V [b)] 0,15 MHz – 80 MHz 6 V [b)] in ISM bands between 0,15 MHz and 80 MHz 80 % AM at 1 kHz

a) The following apply:

- All PATIENT-COUPLED cables shall be tested, either individually or bundled
- PATIENT-COUPLED cables shall be tested using a current clamp unless a current clamp is not suitable. In cases were a current clamp is not suitable, an EM clamp shall be used.
- No intentional decoupling device shall be used between the injection point and the PATIENT COUPLING POINT in any case.
- Testing may be performed at other modulation frequencies identified by the RISK MANAGEMENT PROCESS.
- Tubes that are intentionally filled with conductive liquids and intended to be connected to a PATIENT shall be considered to be PATIENT-COUPLED cables.
- If the frequency stepping skips over an ISM or amateur radio band, as applicable, an additional test frequency shall be used in the ISM or amateur radio band. This applies to each ISM and amateur radio band within the specified frequency range.
- The ISM (industrial, scientific and medical) bands between 0,15 MHz and 80 MHz are 6,765 MHz to 6,795 MHz; 13,553 MHz to 13,567 MHz; 26,957 MHz to 27,283 MHz; and 40,66 MHz to 40,70 MHz. The amateur radio bands between 0,15 MHz and 80 MHz are 1,8 MHz to 2,0 MHz, 3,5 MHz to 4,0 MHz, 5,3 MHz to 5,4 MHz, 7 MHz to 7,3 MHz, 10,1 MHz to 10,15 MHz, 14 MHz to 14,2 MHz, 18,07 MHz to 18,17 MHz, 21,0 MHz to 21,4 MHz, 24,89 MHz to 24,99 MHz, 28,0 MHz to 29,7 MHz and 50,0 MHz to 54,0 MHz.

b) r.m.s., before modulation is applied

c) Discharges shall be applied with no connection to an artificial hand and no connection to PATIENT simulation. PATIENT simulation may be connected after the test as needed in order to verify BASIC SAFETY and ESSENTIAL PERFORMANCE.

12.6 SIGNAL INPUT / OUTPUT PARTS PORT [1]

Phenomenon	Basic EMC standard	IMMUNITY TEST LEVELS
		Professional healthcare facility environment
ELECTROSTATIC DISCHARGE [e)]	IEC 61000-4-2	± 8 kV contact ± 2 kV, ± 4 kV, ± 8 kV, ± 15 kV air
Electrical fast transients / bursts [b) f)]	IEC 61000-4-4	± 1 kV 100 kHz repetition frequency
Surges Line-to-ground [a)]	IEC 61000-4-5	± 2 kV
Conducted disturbances induced by RF fields [b) d) g)]	IEC 61000-4-6	3 V [h)] 0,15 MHz – 80 MHz 6 V [h)] in ISM bands between 0,15 MHz and 80 MHz [i)] 80 % AM at 1 kHz [c)]

a) This test applies only to output lines intended to connect directly to outdoor cables.

b) SIP/SOPS whose maximum cable length is less than 3 m in length are excluded.

c) Testing may be performed at other modulation frequencies identified by the RISK MANAGEMENT PROCESS.

d) Calibration for current injection clamps shall be performed in a 150 Ω system.

e) Connectors shall be tested per 8.3.2 and Table 4 of IEC 61000-4-2:2008. For insulated connector shells, perform air discharge testing to the connector shell and the pins using the rounded tip finger of the ESD generator, with the exception that the only connector pins that are tested are those that can be contacted or touched, under conditions of INTENDED USE, by the standard test finger shown in Figure 6 of the general standard, applied in a bent or straight position.

f) Capacitive coupling shall be used.

g) If the frequency stepping skips over an ISM or amateur radio band, as applicable, an additional test frequency shall be used in the ISM or amateur radio band. This applies to each ISM and amateur radio band within the specified frequency range.

h) r.m.s., before modulation is applied.

i) The ISM (industrial, scientific and medical) bands between 150 kHz and 80 MHz are 6,765 MHz to 6,795 MHz; 13,553 MHz to 13,567 MHz; 26,957 MHz to 27,283 MHz; and 40,66 MHz to 40,70 MHz. The amateur radio bands between 0,15 MHz and 80 MHz are 1,8 MHz to 2,0 MHz, 3,5 MHz to 4,0 MHz, 5,3 MHz to 5,4 MHz, 7 MHz to 7,3 MHz, 10,1 MHz to 10,15 MHz, 14 MHz to 14,2 MHz, 18,07 MHz to 18,17 MHz, 21,0 MHz to 21,4 MHz, 24,89 MHz to 24,99 MHz, 28,0 MHz to 29,7 MHz and 50,0 MHz to 54,0 MHz.

12.7 NOTES TO SECTIONS 13.2 - 13.6

1. 60601-1-2 © IEC:2014

13 INDEX

A

Appendix: guidance, electromagnetic emissions 22

B

Back angle range 12

C

CAUTION statement, significance 4
Certification 19
Cleaning 18
Component Identification 6
Contraindications to intended use 3

D

DANGER statement, significance 4
Disposal 19
Duty cycle 10

E

Electrical requirements, installation 8
Electromagnetic compatibility (EMC) information 5
Electromagnetic emissions, guidance and manufacturer's declaration 21
Electromagnetic interference 8
Exam table weight capacity 10

F

Features 6
Foot control, optional, functions 11

H

Hand pendant functions 11
Height range 12
High-low operation 10

I

Info statement, significance 4
Installation 8
Intended use 3
Introduction 3
Inspection 7

L

Legrest and procedure tray 14
Leveling the exam table 9
Lubrication 17

M

Maintenance 17

N

Notes to section 13 26
NOTICE statement, significance 4

O

Operation 9
Operation safety 9

P

Patient assist arm 14
Pelvic tilt operation 15
Physician's assist storage cabinet 13

S

Safety, equipment clearance 9
Safety, personnel clearance 9
Safety precautions 4
Safety statements, significance 4
Specifications 19
Stirrup operation 15
Storage 18
Symbols, key 21

T

Troubleshooting 16

U

Unpacking 7

W

Warnings 5
WARNING statement, significance 4
Warranty, limited 20
Weight capacity, maximum 4

intensa™
by graham-field

Proudly designed, engineered, and assembled in the USA of domestic and globally sourced components.

Manufactured By:
Intensa, Inc. | 1810 S. Elm Street
High Point, NC 27260 | USA
Manufactured in the USA

Intensa, Inc. is a wholly owned subsidiary of GF Health Products, Inc.
© 2026, GF Health Products, Inc. All Rights Reserved.
Intensa is a registered trademark of GF Health Products, Inc.

IN_560-INS-LAB-RevA26

+1 770.368.4700

Information contained herein is subject to change without notice.
The most current and complete product information can be found on our website.

www.intensa.net | www.grahamfield.com

graham field™